



Omnipod® 5 Automated Insulin Delivery System

User Guide

for Insulet-provided Controller and Android smartphones

INDICATIONS FOR USE

The **Omnipod® 5 ACE Pump (Pod)** is intended for the subcutaneous delivery of insulin, at set and variable rates, for the management of diabetes mellitus in persons requiring insulin. The Omnipod 5 ACE Pump is able to reliably and securely communicate with compatible, digitally connected devices, including automated insulin dosing software, to receive, execute, and confirm commands from these devices. The Omnipod 5 ACE Pump is intended for single patient, home use and requires a prescription.

SmartAdjust™ technology is intended for use with compatible integrated continuous glucose monitors (iCGM) and alternate controller enabled (ACE) pumps to automatically increase, decrease, and pause delivery of insulin based on current and predicted glucose values. SmartAdjust™ technology is intended for the management of type 1 diabetes mellitus in persons 2 years of age and older and type 2 diabetes mellitus in persons 18 years of age and older. SmartAdjust™ technology is intended for single patient use and requires a prescription.

The **SmartBolus Calculator** is software intended for the management of diabetes in persons aged 2 and older requiring rapid-acting U-100 insulin. The SmartBolus Calculator calculates a suggested bolus dose based on user-entered carbohydrates, most recent sensor glucose reading (or blood glucose reading if using fingerstick), rate of change of the sensor glucose (if applicable), insulin on board (IOB), and programmable correction factor, insulin to carbohydrate ratio, and target glucose value. The SmartBolus Calculator is intended for single patient, home use and requires a prescription.

COMPATIBLE INSULINS

The Omnipod 5 Automated Insulin Delivery System is compatible with the following U-100 insulins: NovoLog®, Humalog®, and Admelog®.

Some insulin products are labeled for use in any pump that is compatible with the insulins listed above. To see if another insulin not listed above can be used, refer to section 2.2 of the prescribing information for that insulin product.

CONTRAINDICATIONS

The Omnipod 5 System is NOT recommended for people who:

- Are unable to monitor glucose as recommended by their healthcare provider
- Are unable to maintain contact with their healthcare provider
- Are unable to use the Omnipod 5 System according to instructions
- Are taking hydroxyurea and using a Dexcom Sensor as it could lead to falsely elevated sensor glucose values and result in the over-delivery of insulin that can lead to severe hypoglycemia
- Do NOT have adequate hearing and/or vision to allow recognition of all functions of the Omnipod 5 System, including alerts, alarms, and reminders

Device components including the Pod, Sensor, and Transmitter must be removed before Magnetic Resonance Imaging (MRI), Computed Tomography (CT) scan, or diathermy treatment. In addition, the Controller and smartphone should be placed outside of the procedure room. Exposure to MRI, CT, or diathermy treatment can damage the components.



WELCOME TO OMNIPOD® 5

New Omnipod 5 User

Receiving training and understanding the Instructions for Use are needed BEFORE using your new Omnipod 5 System. Follow these steps to get started:

1. Get Started

Visit: omnipod.com/setup to create your account, link your data management accounts, and learn about training options.

2. Receive Training

Learning how to use your Omnipod 5 System the correct way is important for safe and effective use. Different training methods to learn how to use your system are available based on your and your healthcare provider's preferences.

3. Freedom Is Yours!

You'll then be ready to enjoy the benefits and flexibility of your new Omnipod 5 System.

If you have questions, please contact Customer Care at 1-800-591-3455 for support 24 hours a day, 7 days a week.

To access the complete Omnipod 5 System Technical User Guide

At any time while using Omnipod 5, you can access or request the *Omnipod 5 Technical User Guide for iPhone*.

1. Download or print a digital copy:
 - Visit omnipod.com/guides
 - Scan this QR code with your smartphone.



2. Request to receive a free printed copy:
 - Online request form at omnipod.com/guides
 - Call in to request: 800-591-3455



omnipod.com/guides



Contents

Section 1: Omnipod 5 System Overview	8
Section 2: Set Up Your Omnipod 5 App	10
Section 3: Connect the Sensor	12
Dexcom G6	12
Dexcom G7	14
FreeStyle Libre 2 Plus Sensor	17
Section 4: Set Up a New Pod	22
Prepare.	22
Fill the Pod	23
Activate the Omnipod 5 Pod	24
Apply the Pod	26
Section 5: Omnipod 5 System Modes	28
System Modes	28
System States	29
Switch to Automated Mode	33
Tips for Success	34
Section 6: Get to Know the App	36
Omnipod 5 App Home Screen	36
Glucose Trends and Indicators, View Sensor Graph	37
Alarms and Notifications	38
Section 7: Key Insulin Delivery Actions	42
Deliver a Bolus	42
Custom Foods	44
Start the Activity Feature	46
Cancel the Activity Feature	47
Pause Insulin Delivery	48
Editing a Basal Program	49
Additional Basal Programs	50
Set a Temporary Basal Rate	51

Omnipod 5 System Overview

The Omnipod 5 App

- On provided Controller or a compatible smartphone
- Sends commands to the Pod
- Displays glucose and insulin information from the Pod
- Used to issue meal and correction boluses

The Pod

- Delivers insulin to your body
- Receives commands from the Omnipod 5 App
- Receives sensor glucose values from the Sensor
- Sends sensor glucose values to the Omnipod 5 App
- Automatically adjusts insulin delivery in Automated Mode

The Dexcom G6 or Dexcom G7 Sensor

- Sends sensor glucose values to the Pod and to the Dexcom G6 or Dexcom G7 App
- Does not communicate directly with the Omnipod 5 App
- Cannot communicate with a Dexcom receiver while paired with a Pod

You can set up & start your Dexcom Sensor before or after setting up your Omnipod 5 App. Please consult the Dexcom Instructions for Use for more information.

The FreeStyle Libre 2 Plus Sensor

- Sends sensor glucose values to the Pod and Omnipod 5 App
- Sounds alarms in the Omnipod 5 App
- Cannot communicate with another device while used with Omnipod 5

You must scan and start the FreeStyle Libre 2 Plus Sensor with your Insulet-provided Omnipod 5 Controller. The FreeStyle Libre 2 Plus Sensor is compatible only with the Insulet-provided Controller when using Omnipod 5.

Sensor not included

Sensor not included. For Sensor-specific information, refer to the Instructions for Use for your compatible Sensor.




2

Set Up Your Omnipod 5 App

Omnipod 5 App Setup

Before you set up your Omnipod 5 System, choose whether you want to use the Omnipod 5 App on the provided Controller or a compatible personal smartphone. Connectivity to cellular data or Wi-Fi is important when using the Omnipod 5 System. With either device, make sure to connect to your home or work Wi-Fi network. For a list of compatible smartphones, go to omnipod.com/compatibility.

Initial pump therapy settings, provided by your healthcare provider, are needed to set up your Omnipod 5 App.

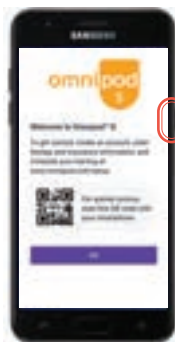

If using the provided Controller as your Controller:

- Hold down the Power button to turn it on.

OR

If using your compatible personal Android smartphone:


- Download the Omnipod 5 App on Google Play.
- Ensure Bluetooth® is turned ON on your compatible smartphone.
- In order to use Omnipod 5 App on a compatible smartphone, you must first log into the Omnipod 5 App on the provided Controller.



- If you plan to use the Omnipod 5 App for iPhone, review the *Omnipod 5 User Guide for iPhone*.

Note:

If you are using the FreeStyle Libre 2 Plus Sensor with Omnipod 5, you must use the Insulet-provided Controller and not a smartphone.

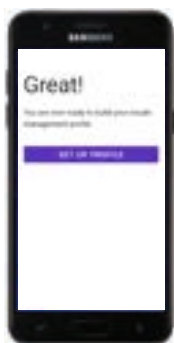

The Omnipod 5 App will guide you through setup. Make sure to read each screen and carefully enter information.

An Omnipod ID is needed for setup. You will be prompted to sign in or be directed to create a new ID.

Setup is complete after entering your personalized initial pump therapy settings (provided by your healthcare provider).




3 Connect the Sensor

Dexcom G6

You must use the Dexcom G6 App on your smartphone to start and stop your Sensor and Transmitter. If you have been using the Dexcom G6 receiver, turn it off. Your Transmitter will not pair with your Pod if it is still connected to the receiver.


Locate your Dexcom G6 Transmitter Serial Number (SN). This can be found in your Dexcom G6 mobile App Settings, on the back of the Transmitter, and on the Transmitter box.

Step 1: Select Dexcom G6 as your Sensor

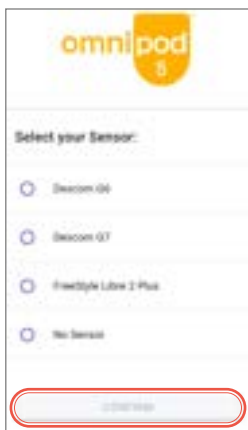

From first time setup select your Sensor.

OR

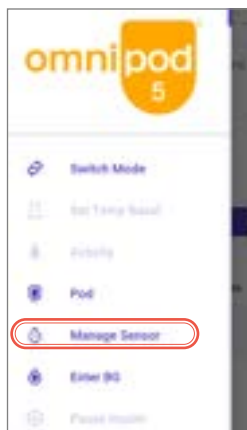

From Home screen.

- Tap the Menu button.
- Tap **Manage Sensor**.
- Select your Sensor.

Step 2: Enter & Save New Transmitter serial number (SN)



- Tap **ENTER NEW**.



- Tap first box to enter Transmitter serial number (SN).



- Tap **DONE**.
- Tap **SAVE**.


Note:

Your Pod uses the SN to connect to the correct Transmitter. You will need to enter a new SN any time you replace your Transmitter.


Dexcom G7

You must use the Dexcom G7 App on your smartphone to start and stop your Sensor. If you have been using the Dexcom G7 receiver, turn it off. Your Sensor will not pair with your Pod if it is still connected to the receiver.

Step 1: Select Dexcom G7 as your Sensor

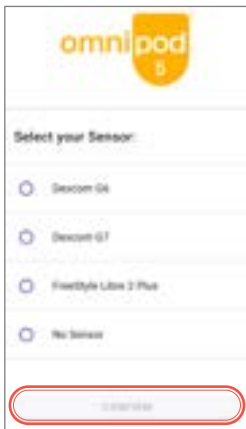

OR

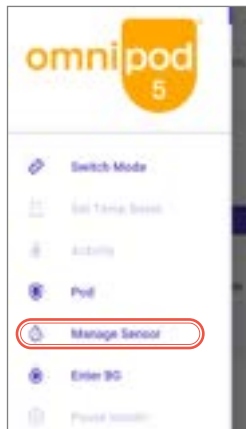

From first time setup select your Sensor.

From Home screen.

- Tap the Menu button.
- Tap **Manage Sensor**.
- Select your Sensor.

Step 2: Enter your Sensor pairing code and serial number



Tap **ADD NEW**.



- To use the Take Photo option to connect, tap TAKE PHOTO.
- To enter the numbers, tap ENTER CODE MANUALLY.

Note: You will need to connect each new Dexcom G7 Sensor to both the Omnipod 5 App and Dexcom G7 App for your Pod and Sensor to stay connected.


Note:

Check that the camera lens is not blocked by your smartphone case or Controller gel skin. You will also need to have camera permission enabled.



Line up the QR code in the green frame, holding both the Controller and applicator steady for several seconds. The photo is taken automatically. It will not be stored.

OR

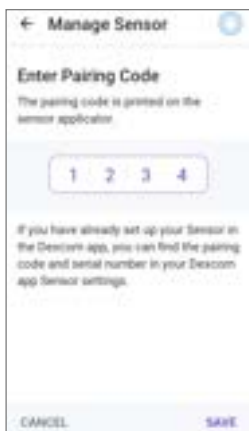

- Enter the 4 digit pairing code on your applicator.
- Tap **SAVE**.



- Enter the 12 digit serial number printed on your applicator.
- Tap **SAVE**.




FreeStyle Libre 2 Plus


All FreeStyle Libre 2 Plus Sensor management is performed in the Omnipod 5 App on the Insulet-provided Controller, including starting a Sensor and configuring and responding to alarms.

If using a FreeStyle Libre 2 Plus Sensor as your Sensor, follow these steps.

Step 1: Select FreeStyle Libre 2 Plus as your Sensor

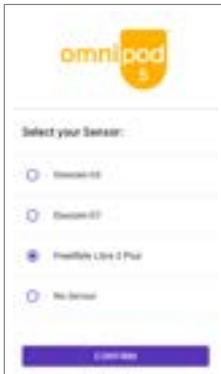

OR

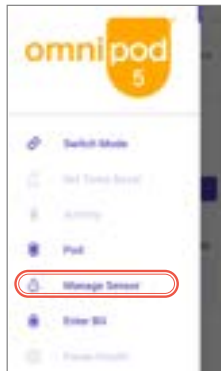


From first time setup select FreeStyle Libre 2 Plus.


From Home screen

- Tap Menu button.
- Tap **Manage Sensor**.

Step 2: Review your Sensor settings

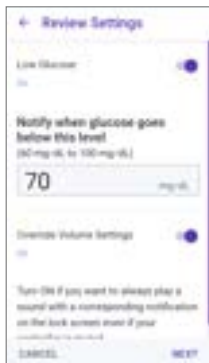

- Review or adjust your Low Glucose setting and volume preferences.
- Tap **NEXT**.

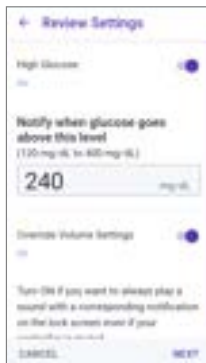


- Review or adjust your High Glucose setting and volume preferences.
- Tap **NEXT**.



- Review or adjust your Missed Sensor Values setting and volume preferences.
- Tap **NEXT**.
- Tap **SAVE**.

Step 3: Apply your FreeStyle Libre 2 Plus Sensor

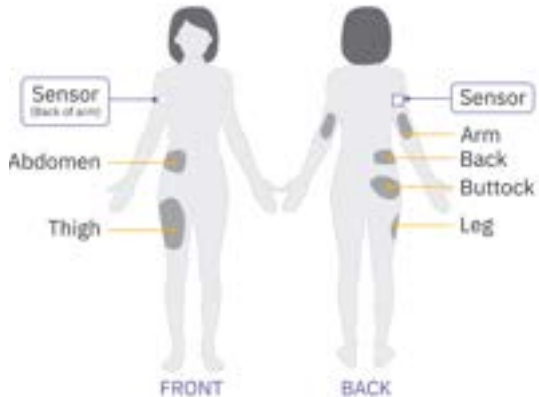

- Follow the on-screen instructions.
- Tap **HOW TO APPLY A SENSOR** if you need help.

Note: Consider these Pod placements to find the locations that work best for your body for optimal line of sight to your Sensor:

- On the same arm 1 inch (2.5 cm) apart
- Abdomen, same side
- Lower back, same side
- Thigh, same side
- Lovehandles, same side
- Upper buttocks, same side
- Back of the opposite arm

Step 4: Scan your Sensor



- Place the back of your Controller up to the Sensor and scan it. The lower third of the Controller should almost touch the Sensor.

- If the Sensor scans successfully, tap **OK**.

It can take up to 20 minutes for the Pod and Sensor to connect.




- After you have started the connection process, you will be asked to switch to Automated Mode.

Switching Between Sensor Types

The Omnipod 5 System is compatible with more than one brand and model of Sensor. If you start the System on one type of Sensor and move to a different Sensor in the future, you can switch your Sensor type from the Manage Sensor screen.

Note: Regular Sensor changes do not require a Pod change, but if you are switching from one brand or model of Sensor to another, you must make this switch between Pod changes. Each Pod can connect to only one type of Sensor.

Step 1: Without an active Pod, tap Switch > from the Manage Sensor screen.

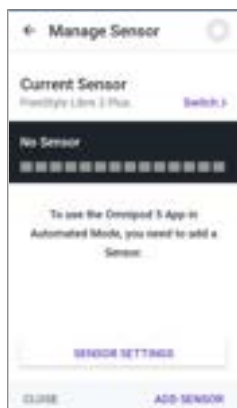

- To change from a FreeStyle Libre 2 Plus Sensor to another brand or model of Sensor, tap **Switch >**.



- To change from a Dexcom Sensor to another brand or model of Sensor, tap **Switch >**.

Step 2: Select your new Sensor brand and model, confirm your new selection, and follow the instructions on the previous pages for first-time set-up of a Sensor. Check the Pod tray lid for Pod and Sensor compatibility.



4 Set Up a New Pod

Prepare

Gather the following supplies:

- Omnipod 5 Controller or smartphone.
- Unopened Omnipod 5 Pod.
- Alcohol prep swabs.
- A vial of room temperature rapid-acting U-100 insulin approved for use with Omnipod 5.

Wash your hands with soap and water.

Clean the top of the insulin vial with an alcohol prep swab.

On the Omnipod 5 App, locate the Pod activation screen.



OR



- After first time setup, tap **SET UP NEW POD**.

- From the POD INFO tab on the Home screen, tap **SET UP NEW POD**.


Fill the Pod

Prepare the fill syringe

- Remove the fill needle and syringe from the Pod's tray. Keep the Pod in its tray during setup. Twist the needle clockwise onto the top of the syringe for a secure fit. Do not use any other type of needle or filling device besides the syringe provided with each Pod.
- Remove the protective needle cap by carefully pulling it straight off the needle.

Fill the syringe

- Gently pull back on the plunger to draw air into the syringe equal to the amount of insulin you will use. You must fill the syringe with at least 85 units of insulin (MIN fill line). Insert the needle into the vial and push the plunger in to inject the air.
- With the syringe still in the vial, turn the vial and syringe upside down. Slowly pull the plunger to withdraw the insulin. Tap or flick the filled syringe to remove any bubbles.

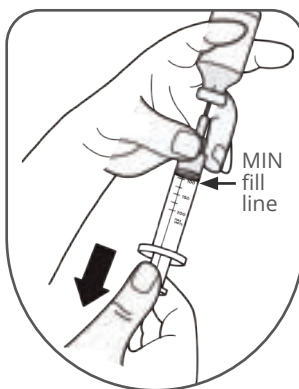

Fill the Pod

- Remove the needle from the vial and insert it straight down into the fill port. An arrow on the white paper backing points to the fill port. Slowly push the plunger down to completely fill the Pod.
- The Pod will beep twice to indicate the Omnipod 5 Pod is ready to proceed.




Activate the Omnipod 5 Pod

- With the Pod still in its tray, place it next to and touching the Controller to ensure proper communication. Tap **NEXT** on the Controller. The system will perform a series of safety checks and automatically primes the Pod.




Pod Placement

Adults and Children

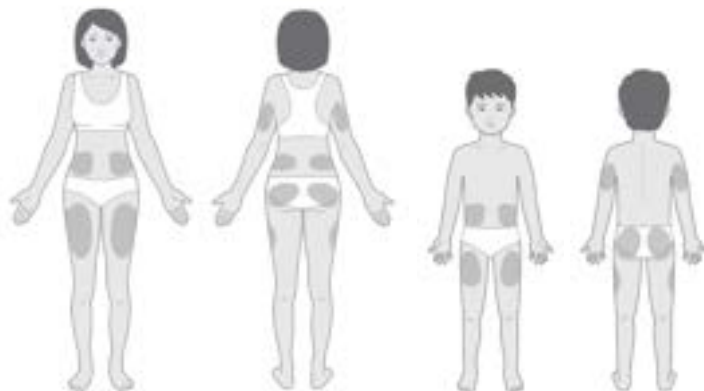

Sensor Placement

The Pod and Sensor should be worn in line of sight, which means worn on the same side of the body in a way that the two devices can “see” one another without your body blocking their communication. Examples shown of various abdomen and arm Sensor placements.

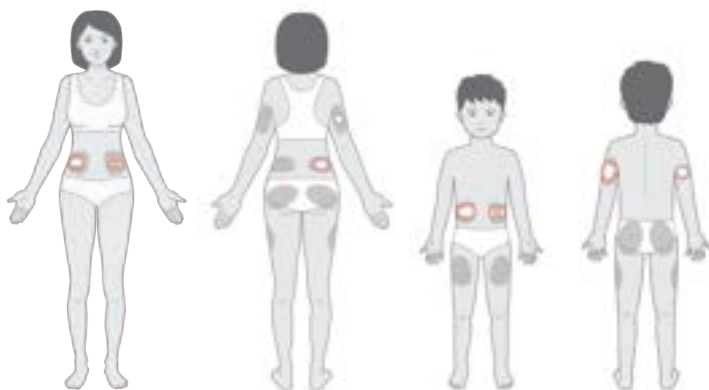

Guidelines for Pod Site Selection

Place your Pod and Sensor as indicated in the Instructions for Use for your compatible Sensor:

- At least 3 inches (8 cm) apart for your Dexcom Sensor.
- At least 1 inch (2.5 cm) apart for your FreeStyle Libre 2 Plus Sensor.
- Place within line of sight of the Sensor for the best connectivity.

Note: Line of sight means that the Pod and Sensor are worn on the same side of the body in a way that the two devices can “see” one another without your body blocking their communication.

- Ideal sites have a layer of fatty tissue.
- Ideal sites offer easy access and viewing.
- The site should be at least 1 inch (2.5 cm) away from the previous site to avoid skin irritation.
- The site should be at least 2 inches (5 cm) away from your navel.
- Avoid sites where belts, waistbands, or tight clothing may rub against or dislodge the Pod.
- Avoid sites where the Pod will be affected by folds of skin.
- Avoid placing the Pod over a mole, tattoo, or scar, where insulin absorption may be reduced.
- Avoid areas of the skin with an active infection.

Apply the Pod

Your Pod is now ready for application and insertion.


- Carefully follow the on-screen instructions.
- Check the infusion site after insertion to ensure that the cannula was properly inserted.



How to Change the Pod



- Tap **POD INFO**.

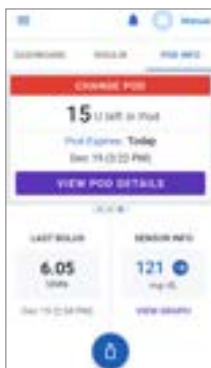

- Tap **VIEW POD DETAILS**.



- Tap **CHANGE POD**.
- Tap **DEACTIVATE POD**.

After the Pod is deactivated, gently lift the edges of the adhesive tab from the skin and remove the entire Pod.

Tip: Remove Pod slowly to help avoid possible skin irritation.

After you have deactivated and removed the old Pod, follow the instructions on how to Activate a Pod in this guide.

DO NOT apply a new Pod until you have deactivated and removed the old Pod.

You may need to change the Pod:

- When the Pod is low on insulin or empty, or the Pod is nearing expiration or expired.
- In response to an alarm.
- If the Pod/cannula has become dislodged.
- If you have glucose of 250 mg/dL or more and ketones are present.
- If you experience elevated glucose.
- As directed by your healthcare provider.
- If, during activation, the Pod fails to beep.

5

Omnipod 5 System Modes

System Modes

The Omnipod 5 System has two operating modes: Automated Mode and Manual Mode.



Automated Mode

- Adjusts every 5 minutes.
- Adapts by updating your total daily insulin with every Pod change.



Manual Mode

- Uses your Basal Program.

System States



Automated Mode: Limited

- Pod is not receiving sensor glucose values.
- System constantly compares Automated Adaptive Basal Rate and Manual Basal Program and uses whichever is lower.



No Pod Communication

- Pod status is unknown.
- Bring Controller or smartphone closer to Pod.

	Manual Mode	Automated Mode
How it works		
Basal Insulin Delivery	Insulin is delivered according to the active Basal Program	Insulin is delivered and adjusted automatically based on sensor glucose values and 60-minute prediction. When sensor glucose values are not available for adjustments, in Automated: Limited, the System constantly compares Automated Adaptive Basal Rate and Manual Basal Program and uses whichever is lower.
Bolus Insulin Delivery	Insulin is delivered using the SmartBolus Calculator or entered manually	Insulin is delivered using the SmartBolus Calculator or entered manually
Connected Sensor	Not required. If connected, sensor glucose values displayed, stored in history, and available for use in SmartBolus Calculator.	Required. Sensor glucose values used for automated insulin delivery, displayed, stored in history, and available for use in SmartBolus Calculator.

	Manual Mode	Automated Mode
What you can do		
Basal Programs	Edit, create new, activate Basal Programs. Does not impact Automated Mode.	Edit Target Glucose to impact automated insulin delivery. Cannot modify Basal Programs in Automated Mode.
Basal Insulin Delivery	Start and cancel Temp Basal rate	Start and cancel the Activity feature
Bolus Calculator Settings	Edit Bolus Settings	Edit Bolus Settings
Bolus Insulin Delivery	Deliver and cancel Immediate and Extended Boluses	Deliver and cancel Immediate Boluses
Pod Changes	Activate and Deactivate Pods	Deactivate Pods When a Pod is deactivated, the System switches to Manual Mode. After you activate a new Pod, you'll be prompted to switch to Automated Mode.
Manage Sensor	View and modify Dexcom G6 Transmitter serial number (SN) or Dexcom G7 pairing code and serial number. Switch between Sensor brands and models (between Pod changes). Start or delete a FreeStyle Libre 2 Plus Sensor, view wear duration, and configure alarms.	View Dexcom G6 Transmitter serial number (SN) or Dexcom G7 pairing code and serial number. View FreeStyle Libre 2 Plus Sensor wear duration and configure alarms.

	Manual Mode	Automated Mode
What you can do		
Pause and Start Insulin	Manually pause insulin for a specified duration of up to 2 hours. Manually Start insulin.	System automatically pauses automated insulin delivery based on sensor glucose value/prediction. Switch to Manual Mode to manually pause insulin delivery.
History Details	Review History Details	Review History Details. Auto Events tab shows microbolus deliveries from Automated Mode.
BG Entry	Enter blood glucose readings to save in History Details	Enter blood glucose readings to save in History Details
How you will be notified	Refer to Sections 2 & 5 of the <i>Omnipod 5 System Technical User Guide</i> for a detailed list of alarms and notifications	

Note: In Automated Mode, your Adaptive Basal Rate will be updated with every Pod change. Adaptive Basal Rate is a continuous baseline that the System can adjust up or down every 5 minutes in response to your sensor glucose values.


For your first Pod, since the System doesn't have any history yet, your total daily insulin and initial Adaptive Basal Rate are estimated from the Basal Program you entered during setup.

Switch to Automated Mode

In Automated Mode, insulin delivery is adjusted based on your sensor glucose values.



- Tap the Menu button on the Home screen.

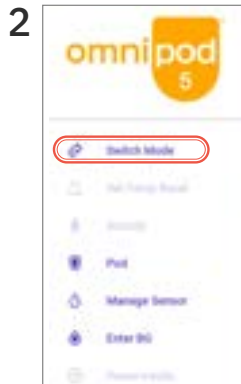

- Tap **Switch Mode**.



- Tap **SWITCH**.
- An active Pod and saved Sensor information within the Omnipod 5 App are required.



- Confirm that the mode switched. Automated should be indicated at the top right of the screen.

Note: Before switching to Automated Mode, an active temp basal, extended bolus, or insulin pause must first be canceled.



Tips for Success

Great things take time

- You can begin using Automated Mode with your first Pod.
- Over time, with every Pod change, Omnipod 5 will adapt to better match your insulin needs.
- Optimizing your insulin delivery could take from a few days to a few weeks, depending on your previous therapy, starting settings, and total daily insulin delivered.

Automated Mode, explained

SmartAdjust™ technology predicts where your glucose will be 60 minutes into the future. You may see the System pause or increase insulin when you are not expecting it if your glucose is predicted to be below or above your Target Glucose setting in the next 60 minutes. To see what the System is doing:

- Check the Sensor Graph: A red bar shows when insulin has been fully paused. An orange bar shows when the System has reached its maximum insulin delivery.
- Check the Auto Events tab in History Detail: This tab shows all automated insulin, both your baseline adaptive basal rate and any adjustment up or down due to your sensor value and trend and/or the 60-minute prediction.

Help your Pod and Sensor stay connected

- If your Pod and Dexcom Sensor lose connection, check your Dexcom App to see if sensor glucose values are available. Confirm the Dexcom G6 Transmitter SN or Dexcom G7 pairing code and serial number match the information in your Omnipod 5 App.
- If you find your System in Automated: Limited often, wear your Pod and Sensor on the same side of the body in a way that the two devices can “see” one another (line of sight) without your body blocking their communication.

Handling highs and lows

There may still be times when you have high or low glucose.

- Give correction boluses to bring down high glucose. This will help the System understand your total daily insulin needs. Try not to override the System's suggestions.
- Use the SmartBolus Calculator whenever you eat. Enter grams of carbs and tap USE SENSOR to calculate a dose based on current sensor value, trend, and Insulin on Board.

Talk to your healthcare provider about:


Treating Lows	Some people find they need to use fewer carbs to treat lows because the System has been decreasing insulin as their glucose drops.
Timing Meal Boluses	Delivering insulin 15–20 minutes before eating could help if you see high glucose after eating.
Adjusting Target Glucose	Decreasing Target Glucose can help the System deliver more automated insulin. Target Glucose is the only setting that you can change to impact automated insulin delivery. Making changes to your basal settings (like your Basal Program or Max Basal) will impact basal insulin delivery only in Manual Mode.
Adjusting Bolus Settings	If you see high glucose after eating, you may need to strengthen your Insulin to Carb ratio to give more insulin for the food you eat. Other bolus settings include Target Glucose, Correction Factor, Duration of Insulin Action, and Reverse Correction. Boluses impact your Total Daily Insulin. Bolusing for meals and to bring down high glucose will help your System learn your insulin needs as it adapts over time.

For more information about treating high and low glucose and handling sick days, see Section 10: Staying Safe with Omnipod 5.

6

Get to Know the App

Omnipod 5 App Home Screen

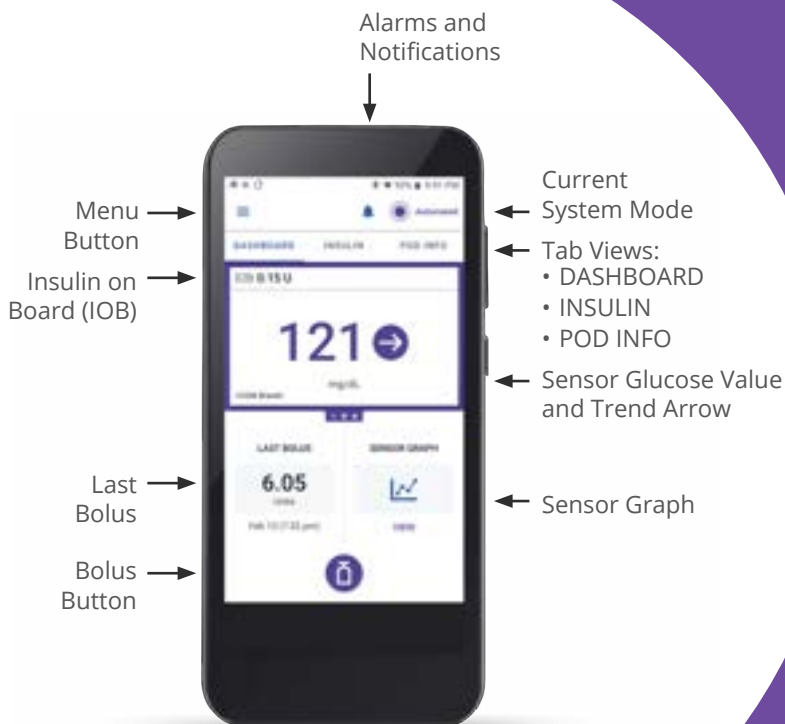

Glucose Trends and Indicators



Automated



Manual

SENSOR GLUCOSE VALUE COLOR KEY:

The sensor glucose value and trend arrow will change color depending on your Glucose Goal Range.

121 →
Trending steady

121 →
Trending steady

68 ↓
Rapidly falling

258 ↗
Slowly rising

■ Sensor glucose value within Glucose Goal Range (Manual Mode)


■ Sensor glucose value within Glucose Goal Range (Automated Mode)

■ Sensor glucose value below Glucose Goal Range (Automated & Manual Modes)


■ Sensor glucose value above Glucose Goal Range (Automated & Manual Modes)

Note: A sensor glucose value will not be displayed if in Limited or No Pod Communication states


View Sensor Graph

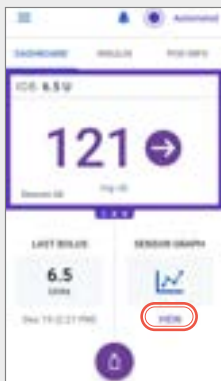

- Tap **VIEW** on Sensor Graph.

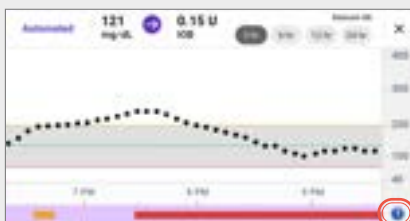

- Tap the question mark icon to view the Graph Legend.

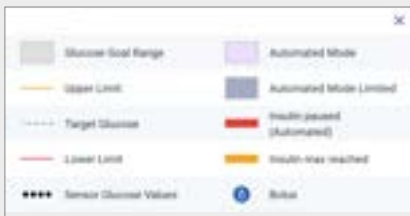

- Sensor Graph Legend.

Note: Sensor Graph differs slightly in appearance depending on Mode.

Alarms and Notifications

The Omnipod 5 System generates different types of alarms and notifications. Alarms repeat every 15 minutes until acknowledged. Alarms that sound on the Pod must be acknowledged in the Omnipod 5 App.



Hazard Alarms

Hazard alarms are high-priority alarms that indicate a serious problem has occurred, and you may need to remove your Pod.

Hazard alarms related to the App

Omnipod 5 App Error	The System detected an error with the App. The Controller may restart.
Omnipod 5 Memory Corruption	The System detected an error with the App. The Controller will be reset. All settings will be deleted. Remove your Pod.
System Error	The System detected an error with the App. Remove your Pod.

Hazard alarms related to the Pod

Blockage Detected	The System detected a blockage (occlusion) in the Pod's cannula. Insulin delivery has stopped. Remove your Pod.
Pod Error	The System detected an error with the Pod. Insulin delivery has stopped. Remove your Pod.
Pod Expired	The Pod has reached the end of its operating life. Insulin delivery has stopped. Remove your Pod.
Pod Out of Insulin	The Pod is empty. Insulin delivery has stopped. Remove your Pod.
Pod Shut-Off	The Pod has stopped delivering insulin because you have set a Pod Shut-off time and did not respond to the Pod Shut-off Advisory alarm. Insulin delivery has stopped. Remove your Pod.

Advisory Alarms

Advisory alarms are lower-priority alarms that indicate that a situation exists that needs your attention. Advisory alarms may escalate to a Hazard alarm.

Advisory alarms related to the Pod

Low Pod Insulin	The amount of insulin in your Pod is below the value you specified in Settings. Escalates to Pod Out of Insulin Hazard alarm if ignored. Change your Pod soon.
Pod Expired	The Pod has expired and will stop delivering insulin soon. Will sound once per hour until it escalates to Pod Expired Hazard alarm. Change your Pod soon.
Pod Shut-Off	The Pod will stop delivering insulin soon because of the Pod Shut-off time you specified in Settings. Tap OK to acknowledge and avoid escalating to Pod Shut-Off Hazard Alarm.
Start Insulin	The time period you specified to pause insulin has ended. Tap START INSULIN to restart insulin and avoid hyperglycemia.

Advisory alarm related to Glucose

Urgent Low Glucose	Your sensor glucose value is 55 mg/dL or below. Consider eating fast-acting carbs to treat hypoglycemia.
--------------------	--

Advisory alarms related to Automated Mode

Missing Sensor Values	In Automated Mode, the Pod has not received sensor glucose values for an hour. The System will operate in Automated: Limited until new values are received.
Automated Delivery Restriction	In Automated Mode, the System has been working to bring your glucose into range but has not seen your glucose change the way it expected. This alarm can let you know to step in and check your Sensor, your Pod, and your glucose. Switch to Manual Mode for 5 minutes or longer to acknowledge this alarm.

Optional, adjustable alarms related to the FreeStyle Libre 2 Plus Sensor

High Glucose	Your sensor glucose value is above your High Glucose setting. Optional alarm will repeat every 5 minutes until your glucose is below the setting or you acknowledge the notification.
Low Glucose	Your sensor glucose value is below your Low Glucose setting. Optional alarm will repeat every 5 minutes until your glucose is above the setting or you acknowledge the notification.
Missing Sensor Values	Sensor glucose values have not been received from your FreeStyle Libre 2 Plus Sensor for 20 minutes. Optional alarm will repeat every 5 minutes, up to 5 times, until sensor glucose values return or you acknowledge the notification.

Problem messages related to the FreeStyle Libre 2 Plus Sensor

Sensor Too Cold	Your Sensor is too cold to provide a glucose value. Move to a warmer location.
Sensor Too Hot	Your Sensor is too hot to provide a glucose value. Move to a cooler location.
Temporary Sensor Problem	Your Sensor is temporarily unable to send sensor glucose values to the Pod or Omnipod 5 App. Check again in 10 minutes.
Sensor Error	Sensor glucose is unavailable. Occurs early in Sensor wear when values are unable to be confirmed as accurate. Tap NEED HELP .
Sensor Ended	Your Sensor has ended. Replace your Sensor.
No Sensor	No Sensor is detected. To use the Omnipod 5 System in Automated Mode, you need to add a Sensor and have an active Pod on.
Replace Sensor	The System has detected a problem with your Sensor that cannot be fixed. Replace your Sensor.
Failed to Connect	Your Sensor did not connect to the Pod. Try again.

Notifications

Action item notifications are for technical System tasks that need your attention, such as App settings or updates. Reminder notifications are related to diabetes management actions you may want to perform.

7

Key Insulin Delivery Actions

Deliver a Bolus



Automated




Manual

Note: USE SENSOR button is active only when Omnipod 5 is receiving a sensor glucose value and trend.


Note: Extended Bolus is available only in Manual Mode.

1

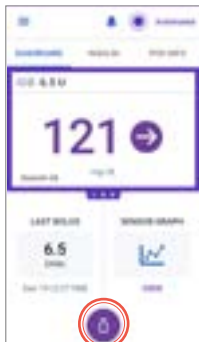

- Tap the Bolus button on the Home screen.

2

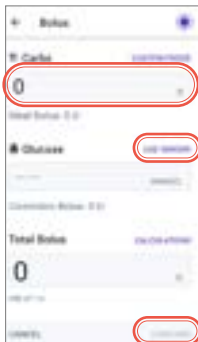

- Tap on the Carbs field to manually enter carbs.
- Tap **USE SENSOR** to use sensor glucose value and trend or add blood glucose reading by tapping the Glucose field.
- Tap **CONFIRM**.

3



- Review entries are correct.
- Tap **START** to begin bolus insulin delivery.

4



- Home screen will display progress of bolus delivery.
- To cancel a bolus in progress, tap **CANCEL**.



Note:

Always bolus for meals as directed by your healthcare provider. In Automated Mode, bolus doses still require your programming and delivery. Failure to deliver a bolus for meals could lead to hyperglycemia.

Custom Foods

Omnipod 5 allows you to save carb information for certain favorite foods, snacks or meals (Custom Foods) that you might eat frequently.

To create or edit a Custom Food, tap Custom Foods from the Menu.

1



- Tap **ADD**.
- Enter a name and tap **Done**.
- Enter a carb count and tap **Done**.
- Tap **SAVE**.

2



- You will see a green badge that reads **NEW** next to your new entry.



3



- Tap **EDIT** to edit your list. You can drag to reorder items, delete items or tap them to edit.

To use Custom Foods for a bolus, tap Custom Foods on the SmartBolus Calculator screen.

During a bolus, you can sort foods using the up-down arrow button and add them to your bolus.

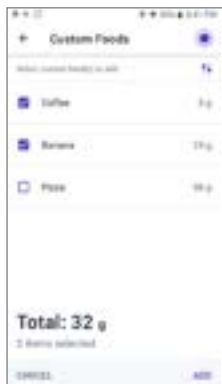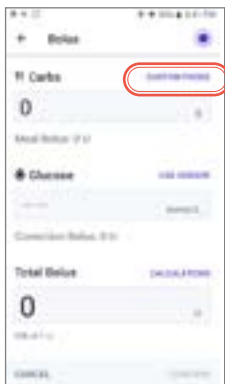

- You can choose which foods to add to your calculation. Tap **ADD**.

Start the Activity Feature




Note: The Activity feature is available only in Automated Mode

The Activity feature of the Omnipod 5 System can be enabled for times when there may be a decrease in insulin needs, like exercise. It will set the Automated Mode Target Glucose to 150 mg/dL and reduce insulin delivery.

Note: The Activity feature does not change the Target Glucose used in bolus calculations.




- Tap the Menu button on the Home screen.

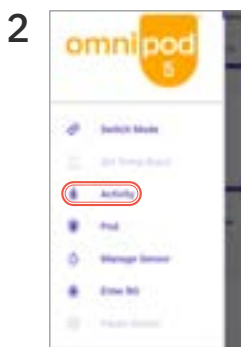

- Tap **Activity**.




- Set Duration (1-24 hrs).
- Tap **CONFIRM**.

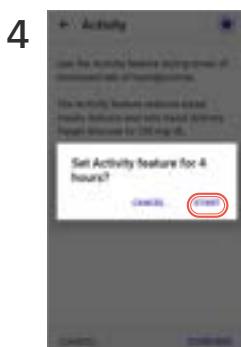

- Tap **START**.

Omnipod 5 App screens are for educational purposes only. Consult your healthcare professional before using these features and for personalized recommendations.

5

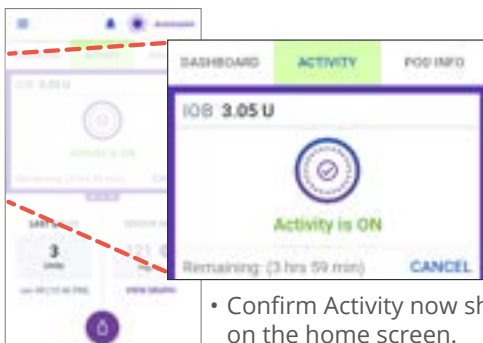

- Confirm Activity now shows on the home screen.


Cancel the Activity Feature



Automated


You can cancel the Activity feature at any time. Upon cancellation or expiration of the defined time period, full automated basal delivery starts on its own, and the Omnipod 5 System returns to using the user-defined Target Glucose.

1

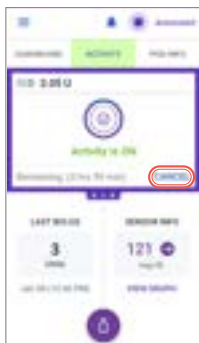

- Tap **CANCEL** on the ACTIVITY Tab.

2

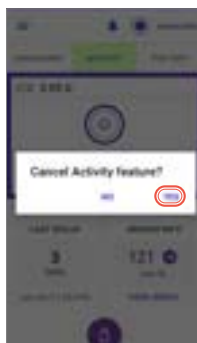


- Tap **YES**.


Pause Insulin Delivery



- Tap the Menu button on the Home screen.

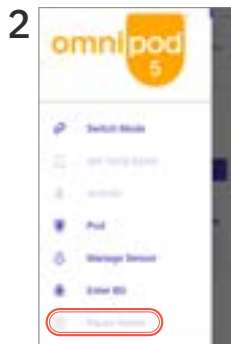


- Tap **Pause Insulin**.

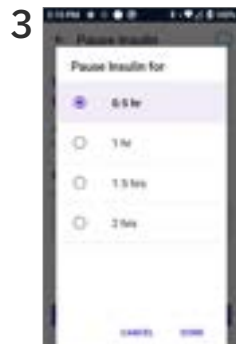


- Use scroll wheel to tell the System how long you'd like to pause insulin for.


Start Insulin Delivery

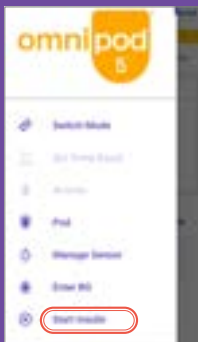

- Tap **Start Insulin**
- Follow the Menu instructions to start insulin

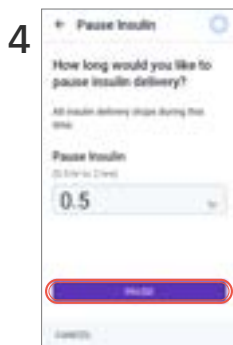

- Tap **PAUSE**.

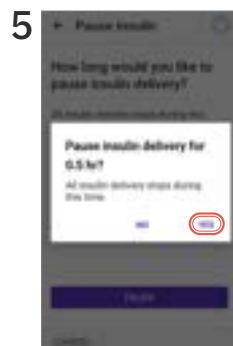

- Tap **YES** to confirm insulin pause.

Insulin delivery does not automatically start at the end of the paused period. You must tap **START INSULIN** to start insulin delivery.


Editing a Basal Program

On occasion, you and your healthcare provider might want to update your basal program to better reflect your current insulin needs.

Note: Editing a Basal Program will NOT affect Automated Mode insulin delivery. To edit a Basal Program, you must be in Manual Mode, and the changes will impact only Manual Mode.



- Tap the **INSULIN** tab on the Home screen.
- Tap **VIEW**.

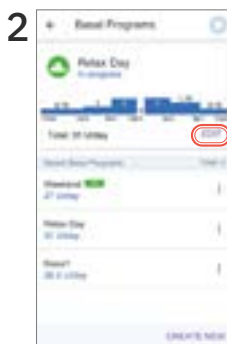

- Tap **EDIT**.



- Tap **YES**.




- Tap to edit program name or tap **NEXT** to edit basal time segments and rates.

5



- Tap the time segment to edit.
- Tap **SAVE** after confirming edits in the basal program.

6

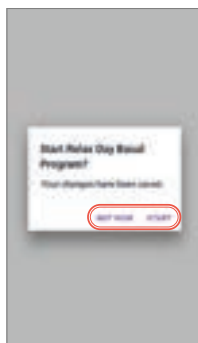

- To start the Basal Program now tap **START**. Otherwise tap **NOT NOW** to save to use at a later time.



Additional Basal Programs

Some people have additional basal programs to help with varying routines, like weekends or work days. These can be used only in Manual Mode.

- Additional Basal Programs can be created by navigating to the Menu button > Basal Programs and tapping **CREATE NEW**.
- Tap the Program Name field to enter a descriptive name for the new Basal Program.
- Tap **NEXT** and define the basal segments one at a time.


Set a Temporary Basal Rate

On occasion, you might want to temporarily change your basal rate for illness or activity.

Note: Temp Basal is available only in Manual Mode.



- Tap the Menu button on the Home screen.

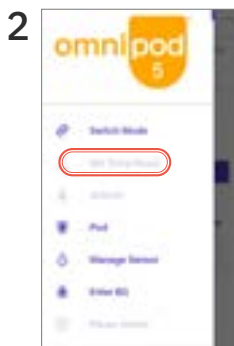

- Tap **Set Temp Basal**.



- Tap Basal Rate entry box and select % change.

Note: The up arrow indicates an increase. The down arrow indicates a decrease.



- Review selections are correct and tap **START**.



- Tap **START**.

- Tap **DURATION** entry box and select time duration.
- Tap **CONFIRM**.

omnipod

5

For More Information

Please refer to your Omnipod[®] 5
Automated Insulin Delivery System
Technical User Guide



Visit us online at
omnipod.com/guides



Insulet Corporation

100 Nagog Park

Acton, MA 01720

1-800-591-3455 | 1-978-600-7850

Controller FCC ID: 2ADINN5004L

Controller FCC ID: 2ADINN5004LR1

Pod FCC ID: RBV-029

Pod FCC ID: RBV-029C

Pod FCC ID: RBV-029D

Medical Disclaimer: This handout is for information only and is not a substitute for medical advice and/or services from a healthcare provider. This handout may not be relied upon in any way in connection with your personal health care related decisions and treatment. All such decisions and treatment should be discussed with a healthcare provider who is familiar with your individual needs.

© 2023-2024 Insulet Corporation. Insulet, Omnipod, the Omnipod logo, and SmartAdjust are trademarks or registered trademarks of Insulet Corporation. All rights reserved. The Bluetooth word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. and any use of such marks by Insulet Corporation is under license. Dexcom, Dexcom G6, and Dexcom G7 are registered trademarks of Dexcom, Inc. and used with permission. The sensor housing, FreeStyle, Libre, and related brand marks are marks of Abbott and used with permission. All other trademarks are the property of their respective owners. The use of third-party trademarks does not constitute an endorsement or imply a relationship or other affiliation.

Patent information at www.insulet.com/patents.

PT-002112-AW Rev 02 11/24

Reference number: PDM-H001-G-MG



PT-002112